


# TFF: Permeate line



With: Bioclamp, pressure sensor, UV sensor, Valve, Flow sensor

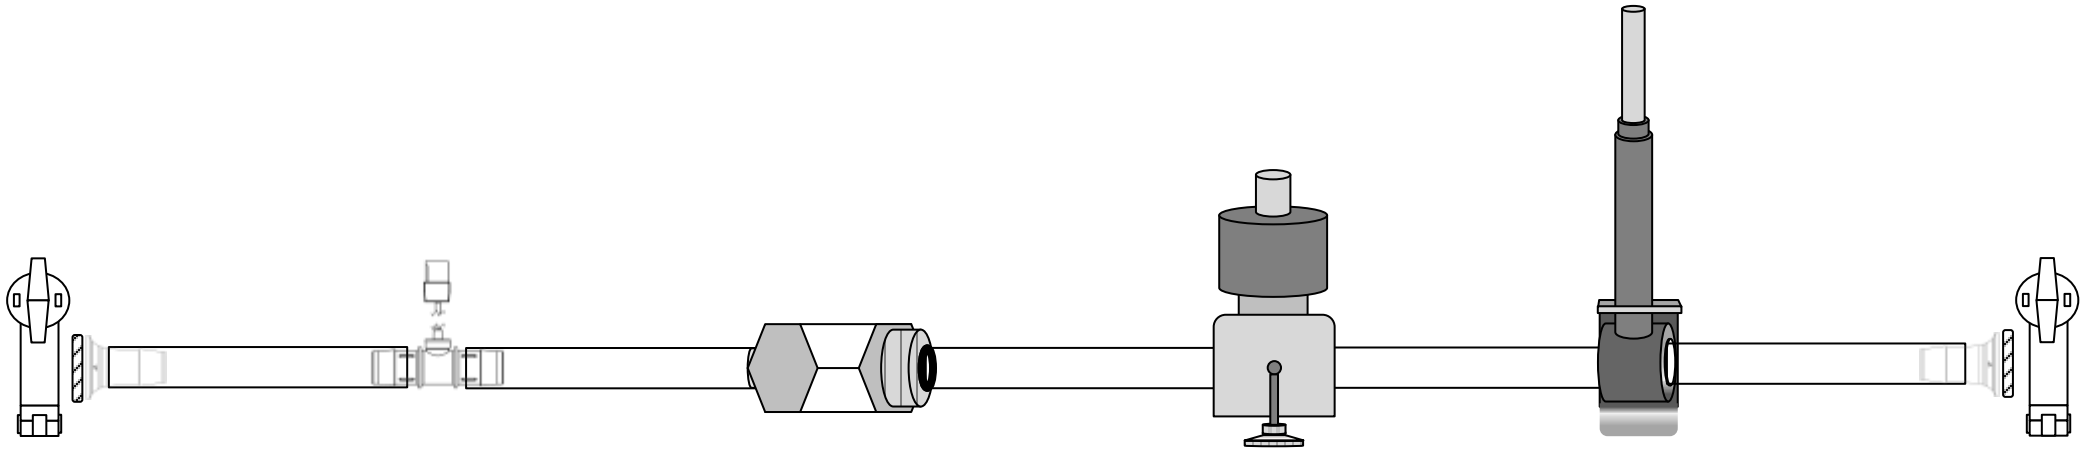

## CUSTOMER APPROVAL READ & APPROVED:

Name: \_\_\_\_\_

Date: \_\_/\_\_/\_\_

Signature: \_\_\_\_\_

## Info on Packaging & Gamma Irradiation

Packaging: double bagged

Label: on outside bag

Gamma Irradiation: Yes, 25-40kGy

## Bill of Materials

All connections, unless otherwise specified, are reinforced with single cable ties

This document is the property of Hitma UltraPure B.V. and must not be disclosed to third party without the written consent of Hitma UltraPure B.V. .This drawing represents the components only schematically to illustrate the function and/or assembly of the equipment/device and to enable the customer to check the component's completeness. The semblance of the real components may therefore deviate from the drawing.